

KUPNÍ SMLOUVA

podle §2079 a násl. občanského zákoníku č. 89/2012 Sb. v platném znění

Článek 1. SMLUVNÍ STRANY

Kupující :

Mikrobiologický ústav AV ČR, v.v.i.
Vídeňská 1083, 142 20 Praha 4
IČ: 61388971, DIČ CZ61388971
Bankovní spojení: Komerční banka
číslo účtu: 2866660287/0100
Zastoupený: Ing. Jiří Hašek, CSc. - ředitel
Zapsaný v rejstříku veřejných výzkumných institucí vedených MŠMT

Prodávající:

AP Czech, s.r.o.
Vacínova 536/3, Praha 8, 180 00
IČ: 26134144
DIČ: CZ26134144
Bankovní spojení: UniCredit Bank, a.s.
č. účtu: 4794004/2700
zastoupený: Ing. Jakub Dubravec, jednatel
Společnost zapsána v obchodním rejstříku vedeném u Městského soudu
v Praze, spisová značka C 73200

uzavřely níže uvedeného dne, měsíce a roku v důsledku skutečnosti, že nabídka prodávajícího byla kupujícímu vybrána ve výběrovém řízení veřejné zakázky s názvem „Víceúčelové zobrazovací zařízení pro molekulární biologii“ jako nabídka nejvhodnější tuto

kupní smlouvu

Článek 2. PŘEDMĚT SMLOUVY

- 2.1 Předmětem smlouvy je koupě přístroje Amersham Typhoon 5 (dále jen přístroj) dle technické specifikace, která je jako Příloha č. 1 nedílnou součástí této smlouvy.
- 2.2 Prodávající je povinen na své náklady dopravit přístroj do laboratoře určené kupujícím (Vídeňská 1083, Praha 4), přístroj zapojit, předvést a odzkoušet a zaškolit zaměstnance kupujícího s obsluhou přístroje.

Článek 3. KUPNÍ CENA A PLATEBNÍ PODMÍNKY

- 3.1 Kupní cena za přístroj je stanovena dohodou smluvních stran a činí 3 791 402,06 Kč bez DPH, DPH ve výši 796 194,45 Kč a kupní cena vč. DPH 4 587 596,51 Kč. Tato cena je konečná, nejvýše přípustná a zahrnuje veškeré náklady prodávajícího s dodáním a instalací přístroje.
- 3.2 Datem zdanitelného plnění je podpis předávacího protokolu kupujícím.
- 3.3 Kupující uhradí kupní cenu na základě faktury prodávajícího po podpisu předávacího protokolu. Faktura musí mít všechny potřebné náležitosti podle platných právních předpisů.

- 3.4 K ceně bude připočtena daň z přidané hodnoty ve výši platné ke dni vystavení daňového dokladu.
- 3.5 V případě prodlení s úhradou uhradí kupující zákonný úrok z prodlení.

Článek 4. POVINNOSTI PRODÁVAJÍCÍHO

- 4.1 Prodávající je povinen dodat přístroj za podmínek stanovených touto smlouvou.
- 4.2 Prodávající je povinen jako součást dodávky přístroje předat kompletní technickou dokumentaci přístroje.
- 4.3 Prodávající se zavazuje zabezpečit jako součást dodávky přístroje instalaci, zahrnující umístění přístroje do prostor určených kupujícím, předvedení provozuschopnosti přístroje, zaškolení obsluhy a odzkoušení funkčnosti přístroje.
- 4.4 Prodávající bere na vědomí, že v souladu s ustanovením § 2 písm. e) zákona č. 320/2001 Sb., o finanční kontrole ve veřejné správě, je včetně jeho případného subdodavatele, osobou povinnou spolupůsobit při výkonu finanční kontroly.
- 4.5 Prodávající bere na vědomí, že poskytovatel dotace, případně jím pověřené subjekty (a případně i další kontrolní orgány podle platných právních předpisů), má v rámci kontroly právo přístupu, a to po dobu 10 let od finančního ukončení programu k dokumentům souvisejícím s realizací zakázky.
- 4.6 Prodávající se zavazuje v místě plnění zachovávat čistotu a pořádek. Prodávající nejdéle do podpisu předávacího protokolu odstraní na své náklady vše nepotřebné k provozu (zejména obaly, zkušební vzorky apod.).
- 4.7 Prodávající odpovídá objednateli za veškeré škody, které mu svou činností způsobil sám anebo prostřednictvím třetích osob, kterých ke své činnosti použil.

Článek 5. POVINNOSTI KUPUJÍCÍHO

- 5.1 Kupující je povinen poskytnout prodávajícímu potřebnou součinnost pro dodání přístroje této smlouvy, zejména předat vyklizené a připravené prostory pro instalaci v termínu požadovaném zadavatelem v dostatečném předstihu.

Článek 6. DODACÍ LHŮTA

- 6.1 Prodávající je povinen dodat přístroj do 8 týdnů od uveřejnění této smlouvy v registru smluv.
- 6.2 Převzetí přístroje do užívání se uskuteční podpisem předávacího protokolu. Za kupujícího je oprávněn předávací protokol podepsat [REDAKCE], nebude-li kupujícím určena osoba jiná.
- 6.3 Podpisem předávacího protokolu přechází vlastnické právo k přístroji na kupujícího.
- 6.4 Pokud bude prodávající v prodlení s dodávkou přístroje, uhradí kupujícímu smluvní pokutu ve výši 1.000,- Kč za každý den prodlení.

Článek 7. ZÁRUČNÍ PODMÍNKY, SERVIS, SOFTWARE PODPORA

- 7.1 Záruční lhůta na přístroj činí 24 měsíců od data podpisu předávacího protokolu (*lhůtu doplní prodávající v souladu se svou nabídkou*).
- 7.2 Záruka se vztahuje na závady způsobené vadou materiálu nebo výrobní vadou. Záruka se nevztahuje na spotřební materiál a závady způsobené nedodržením pokynů uvedených v manuálech k obsluze předmětu smlouvy. Náhradním dílem se rozumí taková součást zařízení, u níž se předpokládá stejná životnost jako u základního přístroje; ostatní části jsou považovány za spotřební materiál.


- 7.3 Délka záruční doby nemůže být podmíněna požadovanými platbami (např. za preventivní prohlídku, pravidelnou kalibraci přístroje, záruční prohlídku apod.). Za požadovanou platbu se nepovažuje výměna částí přístroje v souladu se servisním intervalem stanoveným výrobcem v závislosti na používání přístroje.
- 7.4 Záruční i pozáruční servis pro Českou republiku zajišťuje prodávající.
- 7.5 Běžné závady prodávající odstraní do 5 pracovních dní po nahlášení, v případě výměny některého dílu bude závada odstraněna v termínu domluveném s kupujícím, přičemž doba odstranění by neměla přesáhnout 10 pracovních dnů.
- 7.6 Poruchy bude kupující hlásit elektronickou poštou na adresu apczech@apczech.cz. Ohlašovat poruchy jsou za kupujícího oprávněni také [REDACTED] nebo [REDACTED], nebude-li kupujícím určena osoba jiná.
- 7.7 Záruční a pozáruční opravy přístroje provádí AP Czech s.r.o.
- 7.8 V případě nedodržení doby odstranění poruchy v záruční době uhradí prodávající smluvní pokutu ve výši Kč 500,- za každou započatou hodinu prodlení.
- 7.9 Software podpora činí 60 měsíců od data podpisu předávacího protokolu (*lhůtu doplní prodávající v souladu se svou nabídkou*). Software podporou se rozumí zdarma poskytnutí aktualizací či nových verzí ovládacího softwaru přístroje po celou dobu trvání software podpory.

Článek 8. ZÁVĚREČNÁ USTANOVENÍ


- 8.1 Kupující má právo odstoupit od této kupní smlouvy v případě, že by výdaje, které by měl vynaložit, byly poskytovatelem finančních prostředků či kontrolním orgánem shledány jako neuznatelné. Odstoupení je účinné doručením písemného sdělení prodávajícímu.
- 8.2 Proávající výslovně prohlašuje, že souhlasí s uveřejněním plného znění této smlouvy v souladu s ustanoveními zákona č. 340/2015 Sb., o zvláštních podmínkách účinnosti některých smluv, uveřejňování těchto smluv a o registru smluv (zákon o registru smluv), kromě zveřejnění údajů chráněných jinými právními předpisy. Smluvní strany se dohodly, že odpovědnost za uveřejnění smlouvy v registru smluv nese kupující.
- 8.3 Tato smlouva nabývá platnosti dnem jejího podpisu oběma smluvními stranami a účinnosti dnem uveřejnění v registru smluv.
- 8.4 Veškeré změny této smlouvy jsou možné pouze písemnými dodatky, podepsanými oprávněnými zástupci obou smluvních stran.
- 8.5 Smlouva je vyhotovena ve dvou výtiscích, každý má právní sílu originálu a každá smluvní strana obdrží po jednom výtisku.
- 8.6 Smluvní strany prohlašují, že si smlouvu přečetly, s jejím obsahem souhlasí, což na důkaz souhlasu stvrzují svým podpisem.

V Praze dne 23.7.2020

V Praze dne _____



Ing. Jakub Dubravec
jednatel



Ing. Jiří Hašek, CSc.
ředitel



Imaging systems, software, and accessories

Amersham Typhoon Biomolecular Imager

Amersham™ Typhoon™ Biomolecular Imager (Fig 1) is a new generation of laser scanners that provide you with exceptional data quality through extremely sensitive detection, high image resolution, and a very broad linear dynamic range. These versatile imaging systems support multiple imaging modes, including phosphor imaging, red/green/blue (RGB) and long and short wavelengths of near infrared fluorescence (NIR), as well as optical densitometry (OD) of proteins in stained gels. The Amersham Typhoon 5 model offers a five-laser configuration option with advanced photomultiplier tubes to cover all of these imaging modes. Four other Amersham Typhoon models are available—one for RGB fluorescence/OD measurement/phosphor imaging, one for NIR short/NIR long/Green fluorescence, one for NIR short/NIR long fluorescence, and one for phosphor imaging—so you can choose the best option based on the needs of the system users. Moreover, upgrade paths among different models are available at any time after the installation.

Amersham Typhoon scanners deliver:

- **Versatility:** use one system to image multifluorescent-, radioisotope-labeled, and colorimetric samples on gels, membranes, multiwell plates, culture dishes, glass slides, and tissue sections. The IP model is for phosphor imaging only but can be upgraded.
- **Accurate quantitation:** detect signals from as low as 3 pg of protein and differences across a dynamic range with greater than five orders of magnitude.
- **High resolution:** resolve fine details in your sample with a pixel resolution of as low as 10 μm .
- **High sample throughput:** large scanning area of 40 × 46 cm enables you to simultaneously image up to 20 gels or blots, measuring 10 × 8 cm in size. It is also possible to scan up to 9 multiwell plates in a single scan. This throughput facilitates comparisons among blots and plates, reduces workload, and decreases waiting time. The IP model has a scanning area of 35 × 43 cm, which fits GE's largest imaging plate.



Fig 1. Amersham Typhoon Biomolecular Imagers are versatile, high-performance laser scanners for sensitive and quantitative measurements in a multiuser environment. The image shows the main instrument (right), the Amersham Eraser (top left), on top of the accessory cabinet (bottom left).

- **Flexibility:** modular design allows you to customize the imager for your users' needs. Systems can be adapted with stages, detectors, filters, and lasers. Several upgrade kits are available.
- **Ease of use:** Amersham Typhoon 5, RGB, NIR Plus, and NIR models have auto- and semi auto-scan functions, as well as automatic filter recognition.

The Amersham Typhoon series of scanners provides you with versatile and flexible imaging to precisely quantitate proteins, nucleic acids, and other biomolecules. Amersham Typhoon 5, Amersham Typhoon RGB, Amersham Typhoon NIR Plus, and Amersham Typhoon NIR are variable-mode laser scanners that allow users to easily add or change filters to create new laser and filter combinations (Fig 2).



Fig 2. Users can easily exchange the filters in Amersham Typhoon 5, RGB, NIR Plus, and NIR models. If a new filter is inserted or a filter is changed, the instrument automatically recognizes the filter and updates the control software.

Table 1. Typhoon scanner series comprises five different configurations

	Phosphor imaging	Densitometry (OD)	RGB fluorescence	Near-infrared fluorescence
Amersham Typhoon IP	X	O	O	O
Amersham Typhoon NIR	O	O	O	X
Amersham Typhoon NIR Plus	O	X*	X**	X
Amersham Typhoon RGB	X	X	X	O
Amersham Typhoon 5	X	X	X	X

OD = optical density * Optical density accessory (OD plate) is needed ** Only Green fluorescence channel is included
X: supported O: not supported

All Amersham Typhoon models are versatile laser scanners for precise quantitation of biomolecules in gels, blots, and other sample types. Amersham Typhoon 5 model has the same capabilities as the Amersham Typhoon RGB model, with the addition of near-infrared (NIR) functionality. Amersham Typhoon NIR Plus model has the same NIR fluorescence functionality as the NIR model, with the addition of green fluorescence functionality (Table 1).

Amersham Typhoon models support the following imaging modes:

- Near-infrared fluorescence imaging for NIR fluorescent Western blotting and other applications (Amersham Typhoon 5, NIR Plus, and NIR only; all other models can be upgraded).
- Visible fluorescence imaging in red, green, blue (RGB) channels (Amersham Typhoon 5 and RGB; all other models can be upgraded) to support multiplex fluorescence imaging (e.g., 2D-DIGE).
- Imaging of multiplex RGB fluorescent Western blots, using ECL Plex™ and/or other fluorophore-labeled antibodies (Amersham 5 and RGB, NIR Plus includes green fluorescence, NIR short/long, IP model can be upgraded).
- Phosphor imaging, in which samples containing 3H, 14C, 32P, 33P, 35S (or other sources) are exposed to a storage phosphor screen (imaging plate) (Amersham Typhoon 5, RGB, and IP; all other models can be upgraded).
- Optical densitometry for quantitation of colorimetrically-stained samples (e.g., Coomassie™ blue, silver stain) (Amersham Typhoon 5, RGB, and NIR Plus*; all other models can be upgraded).
*Optical density accessory (OD plate) required
- Chemiluminescence imaging that does not require maximum sensitivity (dark scan function) (Amersham Typhoon 5, RGB, and NIR Plus; all other models can be upgraded); for detection of low abundance proteins we recommend the ImageQuant™ LAS 500 or Amersham Imager 600.

Broad linear dynamic range

Amersham Typhoon scanners provide a broad linear dynamic range in all detection modes, for example when using Cy™5 labeled proteins (Fig 3).

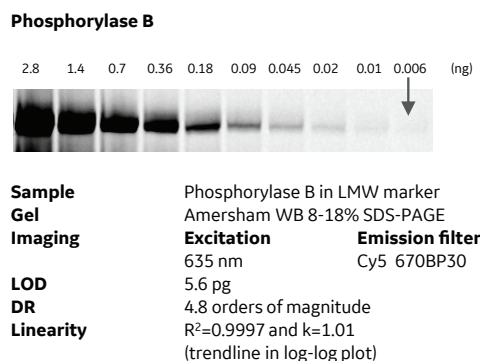
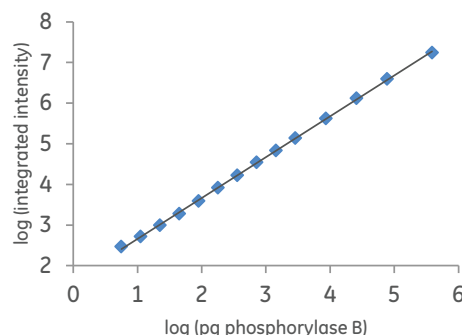


Fig 3. Phosphorylase B was labeled with CyDye™ DIGE fluor Cy5 minimal dye and separated using a precast gradient Amersham WB gel. The gel was imaged with Amersham Typhoon using normal scan speed. A selection of a dilution series is shown in the image; the arrow indicates the limit of detection (LOD). The detection limit was 5.6 pg, and the linear dynamic range (DR) was 4.8 orders of magnitude.

Technical features

Optimal choice of filter, stage, laser and PMT

Amersham Typhoon scanners can house up to eight filters with automatic filter recognition. To attain optimal imaging conditions, you can easily access and exchange emission filters without tools. This feature makes the instrument highly suitable for use in a multiuser environment. In addition to default high performance band-pass filters, there are four open filter positions in which users can put IR-filters, long-pass filters, or custom filters. This next generation of Typhoon scanners feature easier handling of custom filters and a new custom filter box for ease of use.

Stages (Fig 4) give the correct positioning and stability for optimal imaging of a range of sample types. Samples that can be scanned include agarose and polyacrylamide gels, membranes, DIGE gels, microplates, culture dishes, glass slides, and tissue sections. Also, radioisotope-labeled samples can be scanned using a phosphor imaging plate. The system can simultaneously scan two DIGE gels, each measuring up to 21.5 × 27.5 cm, with the multi-stage. Large format sequencing gels (33 × 42 cm) can be scanned using the optional glass stage guide along with the multi-stage. The stages are easily removed from the system for cleaning.

For the detection of radioactivity and fluorescence, emitted light is collected and transformed to an electrical signal by a photomultiplier tube (PMT). The electrical signal is then converted into digital information by A/D conversion for image display and analysis. Amersham Typhoon comes equipped with new bi-alkali and multi-alkali PMTs. This combination provides excellent detection over a very broad spectrum. Each PMT is selected for optimal response to the detected emission wavelength. The bi-alkali PMT is used for phosphor imaging, whereas the multialkali PMT is used for all fluorescence and densitometry imaging modes.

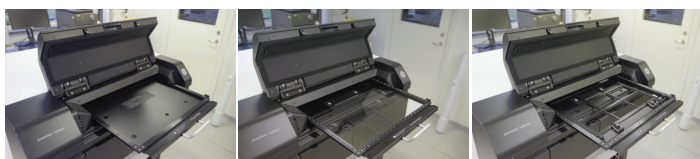


Fig 4. (A) The IP stage, (B) fluor stage, and (C) multi-stage are designed to accommodate a variety of sample formats and imaging modes.

Imaging applications

Amersham Typhoon 5 and RGB enable users to image fluorescent, radiolabeled, and colorimetrically stained gels with a single system.

Fluorescence detection—visible and near-infrared



Upon excitation, light is emitted from a fluorescently labeled sample in proportion to the amount of labeled protein or DNA in the sample. The high sensitivity and broad dynamic range of Amersham Typhoon 5, RGB, NIR Plus, and NIR scanners (Figs 3, 5–9) makes it possible to measure low and high abundant proteins in a single scan.

Multiple fluorescent wavelengths can be detected with minimal cross-talk for comparative expression experiments. See Table 2 for emission filters.

Table 2. Emission filters



Filter*	Wavelength range (nm)	Detection examples
IP	BP390	Phosphorimaging
Cy2 525BP20	515 to 535	Cy2, GFP
Cy3 570BP20	560 to 580	Cy3
Cy5 670BP30	655 to 685	Cy5 ECL Plex Cy5
IRshort 720BP20	710 to 730	Alexa Fluor™ 700, Cy5.5, IRDye™ 680
IRlong 825BP30	810 to 840	Alexa Fluor 790, IRDye 800

* Long pass filters LPB515, LPG550 and LPR660 are available as optional filters.

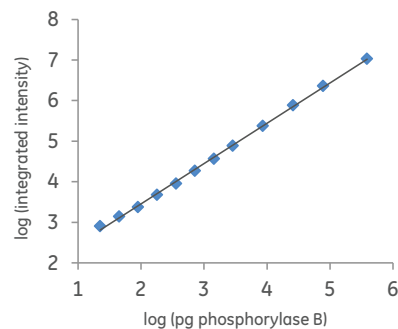


Sample Phosphorylase B in LMW marker
Gel Amersham WB 8-18% SDS-PAGE
Imaging **Excitation** 488 nm **Emission filter** Cy2 525BP20
LOD 22 pg
DR 4.2 orders of magnitude
Linearity $R^2=0.9989$ and $k=0.99$
 (trendline in log-log plot)

Fig 5. Phosphorylase B was labeled with CyDye DIGE fluor Cy2 minimal dye and separated using an Amersham WB electrophoresis gel. The gel was imaged with Amersham Typhoon using normal scan speed. A selection of a dilution series is shown in the image; the arrow indicates the limit of detection (LOD). The detection limit was 22 pg, and the linear dynamic range (DR) was 4.2 orders of magnitude.

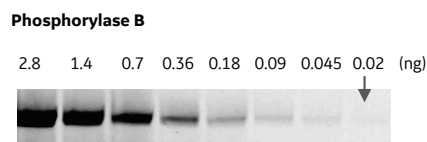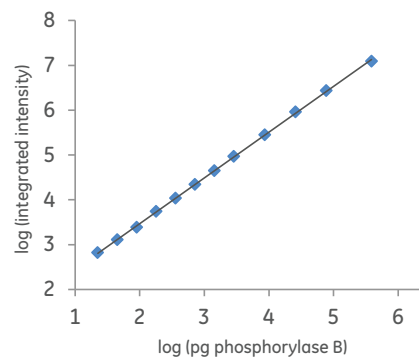


Sample Phosphorylase B in LMW marker
Gel Amersham WB 8-18% SDS-PAGE
Imaging **Excitation** 635 nm **Emission filter** Cy3 570BP20
LOD 22 pg
DR 4.2 orders of magnitude
Linearity $R^2=0.9998$ and $k=1.02$
 (trendline in log-log plot)

Fig 6. Phosphorylase B was labeled with CyDye DIGE fluor Cy3 minimal dye and separated using an Amersham WB electrophoresis gel. The gel was imaged with Amersham Typhoon using normal scan speed. A selection of a dilution series is shown in the image; the arrow indicates the limit of detection (LOD). The detection limit was 22 pg, and the linear dynamic range (DR) was 4.2 orders of magnitude.

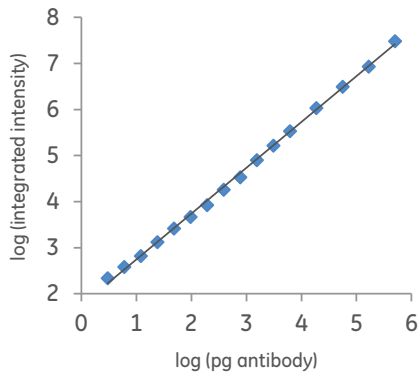


Antibody heavy chain

386 192 96 48 24 12 6 3 (pg)




Sample IRDye™ 680 goat anti-rabbit antibody
Gel Amersham WB 13.5% SDS-PAGE
Imaging **Excitation** 685 nm **Emission filter** 720BP20 (IRshort)
LOD 3 pg
DR 5.2 orders of magnitude
Linearity $R^2=0.9988$ and $k=1.00$
 (trendline in log-log plot)

Fig 7. Antibody conjugated with IRDye 680 was separated using an Amersham WB electrophoresis gel. To reduce noise, the gel was imaged with Amersham Typhoon using slow scan speed. A selection of a dilution series is shown in the image; the arrow indicates the limit of detection (LOD). The detection limit was 3 pg, and the linear dynamic range (DR) was 5.2 orders of magnitude

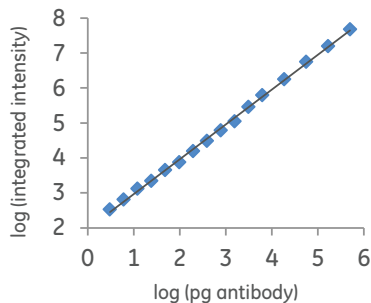

Antibody heavy chain

386 192 96 48 24 12 6 3 (pg)




Sample IRDye 800 goat anti-rabbit antibody
Gel Amersham WB 13.5% SDS-PAGE
Imaging **Excitation** 785 nm **Emission filter** 825BP30 (IRlong)
LOD 3 pg
DR 5.2 orders of magnitude
Linearity $R^2=0.9988$ and $k=1.00$
 (trendline in log-log plot)

Fig 8. Antibody conjugated with IRDye 800 was separated using an Amersham WB electrophoresis gel. To reduce noise, the gel was imaged with Amersham Typhoon using slow scan speed. A selection of a dilution series is shown in the image; the arrow indicates the limit of detection (LOD). The detection limit was 3 pg, and the linear dynamic range (DR) was 5.2 orders of magnitude.

Phosphorylase B

1.2 0.58 0.29 0.15 0.073 0.045 0.018 0.009 0.005 (µg)



Sample Phosphorylase B in LMW marker
Gel ExcelGel™ SDS Gradient 8-18 (GE)
Imaging **Excitation** 488 nm **Emission filter** Cy3 LPG
LOD 5 ng
DR 2.4 orders of magnitude
Linearity $R^2=0.989$


Fig 9. A mixture of proteins (LMW Marker, GE Healthcare) was separated by SDS-PAGE followed by staining with SYPRO™ Ruby Protein Gel Stain. The gel was imaged with Amersham Typhoon using normal scan speed. A selection of a dilution series of Phosphorylase B is shown in the image; the arrow indicates the limit of detection (LOD). The detection limit was 5 ng, and the linear dynamic range (DR) was 2.4 orders of magnitude.

Sensitive multiplex detection of Western blots

The versatile Amersham Typhoon 5, RGB, NIR, and NIR Plus scanners are well suited for imaging of fluorescent Western blot membranes. This method is very sensitive, and the signal is proportional to protein quantity. Moreover, it is possible to detect more than one protein at the same time by means of secondary antibodies labeled with different fluorophores. Amersham Typhoon provides high sensitivity and a broad linear dynamic range, supporting its use for quantitative Western blotting (Fig 10-13).


CHO cell lysate

10 5 2.5 1.25 0.63 (µg total protein)

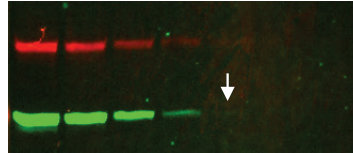


Sample CHO cell lysate with transferrin
Membrane Amersham Hybond™ LFP 0.2 PVDF
Target proteins Transferrin and tubulin
Detection **Primary antibodies** Rabbit anti-human transferrin, Mouse anti-Tubulin
Secondary antibodies Amersham WB Cy5 GAR, IRDye 800 GAM
Imaging **Excitation** 635 nm **Emission filter** Cy5 670BP30
 785 nm 825BP30 (IRlong)
LOD 0.63 µg

Fig 10. Multiplex detection of proteins by Western blotting. Transferrin and endogenous tubulin were targeted in a dilution series of CHO cell lysate using Amersham anti-rabbit Cy5 (red) and anti-mouse IR Dye 800 (green) secondary antibodies. Imaging was performed with Amersham Typhoon scanner. The arrow indicates the limit of detection (LOD) for tubulin. The low background enables reliable quantitation of specific signals relative to a housekeeping protein.

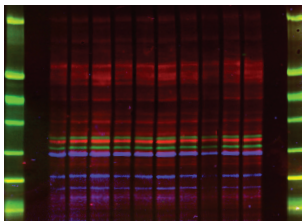


Sample CHO cell lysate
Gel SDS-PAGE 8-18%
Membrane Amersham Hybond P 0.45 PVDF
Detection **Primary antibodies**
 Rabbit anti-ERK
 Mouse anti-GAPDH
Secondary antibodies
 ECL Plex Cy3 GAR
 Alexa Plus 800 GAM
Total protein stain
 Amersham QuickStain™
Imaging **Excitation** **Emission Filter**
 532 nm Cy3 570BP20 (green)
 685 nm IRshort 720BP20 (red)
 785 nm IRLong 825BP30 (blue)

Fig 11. Triplex protein detection with total protein normalization. Different amounts of CHO cell lysate were loaded on an SDS-PAGE gel for Western blot detection. ERK and GAPDH were detected using the 532 nm and 785 nm lasers respectively. Amersham QuickStain labeled total protein for normalization was detected using the 685 nm laser.

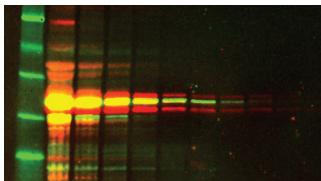

Sample CHO cell lysate, two-fold dilution starting at 40 µg
Gel SDS-PAGE 8-18%
Membrane Amersham Protran™ Premium 0.45 NC
Detection **Primary antibodies**
 Rabbit anti-ERK
 Mouse anti-actin
Secondary antibodies
 Alexa Plus 680 GAM
 Alexa Plus 800 GAR
Imaging **Excitation** **Emission filter**
 685 nm IRshort 720BP20 (green)
 785 nm IRLong 825BP30 (red)

Fig 12. Western blot of a dilution series of CHO cell lysate. Two-plex detection of target protein ERK using Alexa Plus 800 Ab and house-keeping protein actin using Alexa Plus 680 Ab.




Sample CHO cell lysate (lane 1 to 4) with recombinant GST (lane 3 and 4)
Gel SDS-PAGE 8-18%
Membrane Amersham Protran Premium 0.45 NC
Detection **Primary antibodies**
 Rabbit anti-ERK
 Mouse anti-GAPDH and mouse anti-actin
 Goat anti CHO-HCP and goat anti-GST
Secondary antibodies
 Donkey anti-goat DyLight™ 549
 Goat anti-rabbit Alexa™ Plus 680
 Goat anti-mouse Alexa Plus 800
Imaging **Excitation** **Emission Filter**
 532 nm Cy3 570BP20 (green)
 685 nm IRshort 720BP20 (red)
 785 nm IRLong 825BP30 (blue)

Fig 13. Detection of proteins using three different primary antibody species (rabbit, mouse, and goat) is possible with the NIRplus scanner.

2D-DIGE

Amersham Typhoon scanners are designed for use with analysis software such as Melanie™ 9 (Figs 14–16). The strengths of these imaging systems—high sensitivity and broad dynamic range for measuring low and high abundant proteins in one scan—make them highly suited for 2D-DIGE applications, enabling you to detect and accurately quantitate subtle changes in protein expression. By generating overlaid, multichannel images for each gel with minimal cross-talk, Typhoon 5 and Typhoon RGB exploit the multiplexing potential of CyDye DIGE fluors to remove experimental variation between gels. When images are analyzed using high-quality software such as Melanie 9, you will be able to accurately and confidently measure very small differences in protein abundance.

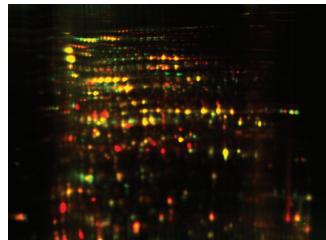

Sample 1 - Cell lysate of *E-coli*
 2 - Cell lysate of *E-coli* treated with benzoic acid
IPG strips 3-10 NL, 24 cm
Gel Precast low-fluorescent DIGE gel
Imaging **Excitation** **Emission filter**
 488 nm Cy2 525BP20
 532 nm Cy3 570BP20
 635 nm Cy5 670BP30

Fig 14. Green/Red-overlay image of a two-dimensional difference gel electrophoresis (2D-DIGE) gel with control and treated samples, and internal standard. The control and treated samples were labeled with Cy3 and Cy5 DIGE Fluors minimal dye labeling protocol. The internal standard sample was labeled with Cy2 DIGE Fluor. The data sets were evaluated using the Melanie™ 2D analysis software, see Fig 15 and 16.

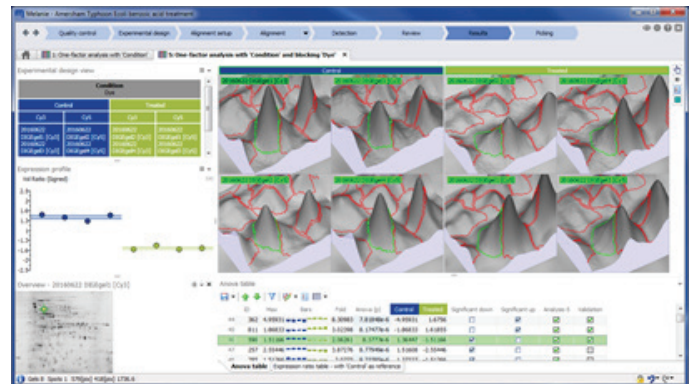


Fig 15. Example of a DIGE experiment analyzed with Melanie 8 (version 8.0.1) software. The effect of benzoic acid treatment on the Escherichia coli proteome was examined. Four replicates each were prepared for the control (blue) and benzoic acid-treated (green) samples, for a total of 8 different samples run on 4 gels. A pooled internal standard was included as a third sample on each gel. The experimental design view (top left) indicates that dye was used as a blocking factor in the statistical analysis. The dye-corrected estimates of the ANOVA p-values further improve the ability to detect subtle but true differences in protein expression, even for overlapping spots. This is shown by the 3-D views of the illustrated protein spot and the corresponding expression profile (middle left).


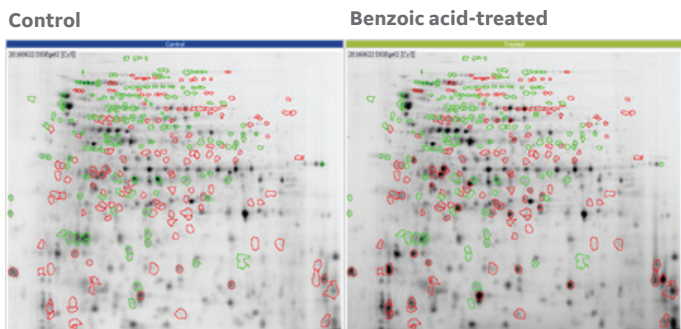


Fig 16. Representative control (blue) and treated (green) gel images of the experiment described in Fig 14 and Fig 15. Spots that are significantly upregulated (p values < 0.001) in the treated group are shown in red; downregulated spots are shown in green.

Fluorescence measurements of biological samples

The large working area of Amersham Typhoon makes it ideally suited for fluorescence investigations of distribution of fluorescent compounds in biological samples. There are numerous different applications, and sample types, which rely on fluorescence as the method of detection. As an example in Figure 17, the distribution of chlorophyll in leaves was measured for multiple samples using different laser and filter combinations and the fluor stage. Popular model organisms that are used to address questions in biology include *Arabidopsis thaliana*, *Drosophila melanogaster*, and *C. elegans*. With the Amersham Typhoon it is easy to measure the two-dimensional distribution of fluorophores in a biological sample, including natural fluorophores, fluorophore-tagged antibodies, and fluorescent proteins.

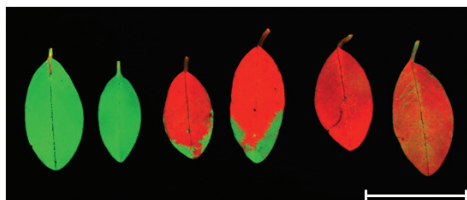


Sample	Green and yellow leaves from <i>Cotoneaster sp.</i>	
Imaging mode	Fluorescence	
Imaging	Excitation	Emission filter
	488 nm	515 nm long-pass (green)
	532 nm	570BP20 (red)

Fig 17. Fluorescence two-color overlay image of green and yellow leaves measured with the Amersham Typhoon scanner. The two leaves in the middle were partly green and partly yellow. Chlorophyll fluorescence can be measured with a long-pass filter and the 488 nm laser. The shift in fluorescence during leaf senescence as a result of chlorophyll loss can be measured with high resolution, in this case with 25 μ m pixel size. The white scale bar is 20 mm. The large working area of the Amersham Typhoon scanner (40 x 46 cm) allows for easy imaging of multiple leaves.

Detection of radioactivity

To detect radioactive signals using phosphor imaging, samples containing radioactive probes are exposed to a storage phosphor screen (imaging plate). Light is emitted from the screen in proportion to the amount of radioactivity in the sample upon laser-induced stimulation (Figs 18-20). All storage phosphor screens from GE are compatible with the Amersham Typhoon scanners.

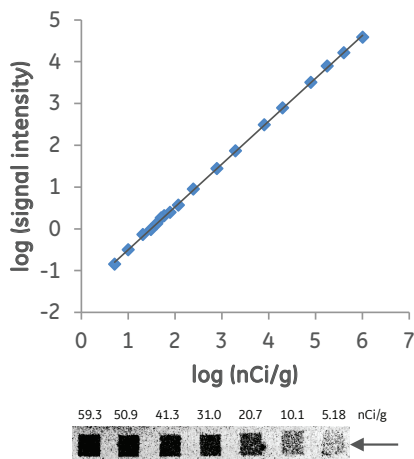

Sample	^{14}C autoradiographic standard (CFQ12000)	
	3 hour exposure to BAS-SR Imaging Plate	
Imaging	Excitation	Emission filter
	635 nm	IP BP390
LOD	0.00518 $\mu\text{Ci/g}$	
DR	5.3 orders of magnitude	
Linearity	$R^2=0.9998$ and $k=1.03$ (trendline in log-log plot)	

Fig 18. Scanned image of a ^{14}C autoradiographic standard using Amersham Typhoon. A selection of the standard is shown in the image; the arrow indicates the limit of detection (LOD). The linear dynamic range (DR) was 5.3 orders of magnitude.


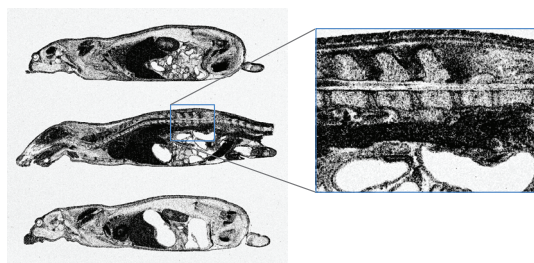


Fig 19. Autoradiography images of rat injected with ^{14}C glucose. The magnified area shows part of the spine. Samples were prepared by Sekisui Medical Co., LTD.

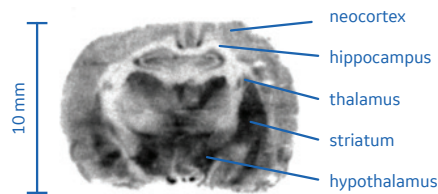

Sample Imaging
 Section of rat brain
Excitation
 635 nm
Emission filter
 IP BP390

Fig 20. Autoradiogram showing the binding of DaTscan™ (123I-ioflupane) to a coronal brain section of rat brain (linear contrast). DaTscan (GE Healthcare) is a SPECT radiopharmaceutical used for dopamine transporter imaging in the diagnosis of Parkinson disease. Sections were incubated with 1 nM DaTscan, in phosphate buffered saline, pH 7.4 (PBS), for 60 min. After incubation was completed, sections were rinsed extensively; 3 x 3 min in cold PBS and dried before being exposed to SR imaging plates (GE Healthcare) for 60 min. The sections were scanned with 25 µm pixel size using the Amersham Typhoon scanner. The scale bar is 10 mm.

Sample preparation by Sergio Estrada, Preclinical PET –MRI Platform, Dept. of Medicinal Chemistry, Uppsala University.

File formats

Data are stored either in linear 16-bit grayscale (.TIF file format), in square root encoded 16-bit (.GEL file format), or log encoded 16-bit (.IMG file format). The .GEL and .IMG formats provide the highest dynamic resolution for fluorescence and phosphor imaging. All file formats are TIF based images and compatible with common image analysis softwares, such as ImageJ (NIH, USA).

Image analysis

Designed for seamless data transfer and quantitative gel and blot analysis, GE provides image analysis software for use with Amersham Typhoon (Table 3).

Table 3. Image analysis software

Software	Analysis
ImageQuant™ TL	1D gel electrophoresis, dot blots, arrays, colony counting, and user-defined gel analysis
Melanie 2D	2D gels, including single stain, 2D-DIGE, and 2D-DIBE for HCP Coverage assay

Densitometry

When using Amersham Typhoon 5 and RGB, excitation light passes through the sample and excites a fluorescent plate. The emitted light from the plate passes through the sample again and is collected and converted to an electrical signal. The method is suitable for documentation of colorimetrically stained gels (Fig 21). These Amersham Typhoon scanners also have optical density measurements for quantitation purposes.

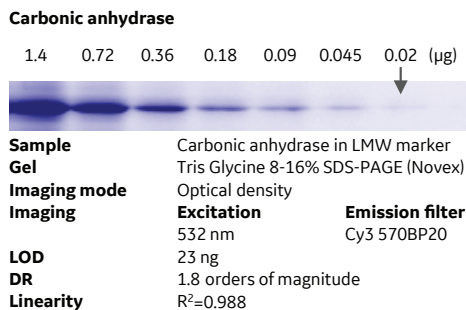


Fig 21. A mixture of proteins (LMW Marker, GE Healthcare) was separated by SDS-PAGE followed by staining with Coomassie Brilliant Blue (G-350). The gel was imaged with Amersham Typhoon in optical density mode. A selection of a dilution series of carbonic anhydrase is shown in the image; the arrow indicates the limit of detection (LOD). The detection limit was 23 ng and the linear dynamic range (DR) was 1.8 orders of magnitude.

Validation support

A comprehensive suite of life cycle validation services is available for laboratory systems used in good practice environments, such as GLP, GMP, or GCP. The documentation is developed and approved by validation experts. Installation Qualification and Operation Qualification (IQ/OQ) are performed on-site by trained service engineers. Our engineers can also help with periodic re-qualification (RQ) and evaluate, verify, and document system changes and software upgrades with Change Control Protocols (CCP).

Product specifications

	Amersham Typhoon 5	Amersham Typhoon RGB	Amersham Typhoon NIR Plus	Amersham Typhoon NIR	Amersham Typhoon IP
Detection modes:	Fluorescence, phosphor imaging, densitometry, and chemiluminescence (Dark scan)	Fluorescence, phosphor imaging, densitometry, and chemiluminescence (Dark scan)	2xNIR and G fluorescence, densitometry*, and chemiluminescence (Dark scan)	2xNIR fluorescence	Phosphor imaging
Laser excitation wavelengths	LD488, SHG532, LD635, LD685, LD785	LD488, SHG532, LD635	SHG532, LD685, LD785	LD685, LD785	LD635
Optional excitation wavelengths:		LD685, LD785	LD 488, LD635	LD 488, SHG532, LD635	LD488, SHG532, LD685, LD785
Radioisotopes:	3H, 11C, 14C, 125I, 18F, 32P, 33P, 35S, 99mTc, and other sources of ionizing radiation	3H, 11C, 14C, 125I, 18F, 32P, 33P, 35S, 99mTc, and other sources of ionizing radiation	none	none	3H, 11C, 14C, 125I, 18F, 32P, 33P, 35S, 99mTc, and other sources of ionizing radiation
Measurable dynamic range:	> 5 orders of magnitude	> 5 orders of magnitude	> 5 orders of magnitude	> 5 orders of magnitude	> 5 orders of magnitude
Bit depth:	16-bit	16-bit	16-bit	16-bit	16-bit
Scanning area:	40 × 46 cm	40 × 46 cm	40 × 46 cm	40 × 46 cm	35 × 43 cm
Pixel sizes:	10, 25, 50, 100, 200 µm, and prescan 1000 µm	10, 25, 50, 100, 200 µm, and prescan 1000 µm	10, 25, 50, 100, 200 µm, and prescan 1000 µm	10, 25, 50, 100, 200 µm, and prescan 1000 µm	10, 25, 50, 100, and 200 µm
Standard filters:	IP 390BP, Cy2 525BP20, Cy3 570BP20, Cy5 670BP30, IRshort 720BP20, IRLong 825BP30	IP 390BP, Cy2 525BP20, Cy3 570BP20, Cy5 670BP30	Cy3 570BP20, IRshort 720BP20, IRLong 825BP30	IRshort 720BP20, IRLong 825BP30	IP 390BP
Optional filters:	Cy2 LPB515, Cy3 LPG550, Cy5 LPR660	Cy2 LPB515, Cy3 LPG550, Cy5 LPR660	Cy3 LPG550	None	None
Sample stages:	Fluor Stage, Multi-Stage, and IP Stage	Fluor Stage, Multi-Stage, and IP Stage	Fluor Stage	Fluor Stage	IP Stage
Dimensions (W × H × D):	900 × 400 × 800 mm	900 × 400 × 800 mm	900 × 400 × 800 mm	900 × 400 × 800 mm	900 × 400 × 800 mm
Weight:	94 kg	93 kg	93 kg	93 kg	92 kg
Line frequency:	50/60 Hz	50/60 Hz	50/60 Hz	50/60 Hz	50/60 Hz
Temperature:	18°C to 28°C	18°C to 28°C	18°C to 28°C	18°C to 28°C	18°C to 28°C
Humidity:	20% to 70% (no condensation)	20% to 70% (no condensation)	20% to 70% (no condensation)	20% to 70% (no condensation)	20% to 70% (no condensation)
Supply voltage:	100 - 240 VAC ± 10%	100 - 240 VAC ± 10%	100 - 240 VAC ± 10%	100 - 240 VAC ± 10%	100 - 240 VAC ± 10%
Power consumption:	Approx. 0.3 kVA	Approx. 0.3 kVA	Approx. 0.3 kVA	Approx. 0.3 kVA	Approx. 0.3 kVA

*Optical density accessory (OD Plate) required.

Minimum computer requirement

OS	Windows® 7 Professional (64-bit) Windows 8.1 Pro (64-bit) Windows 10 Pro (64-bit)
Internal memory	8 GB
Processor	Intel® Core i5 processor
Hard disk	80 GB
USB ports	USB 2.0
Optical drive	DVD-ROM Drive

Please contact your local sales representative for the latest recommended computer configuration.

Ordering information

System	Quantity	Product code
Amersham Typhoon 5	1	29187191
Amersham Typhoon RGB	1	29187193
Amersham Typhoon NIR Plus	1	29264463
Amersham Typhoon NIR	1	29238583
Amersham Typhoon IP	1	29187194

One license of ImageQuant TL software is provided with each model of Amersham Typhoon scanners.

Upgrade kits	Quantity	Product code
AmTyphoon_IP_RGB_Upgrade IP to RGB model upgrade	1	29231384
AmTyphoon_NIR_B_Upgrade NIR to Blue Fluorescent function	1	29348804
AmTyphoon_IP_B_Upgrade IP to Blue Fluorescent function	1	29348736
AmTyphoon_RGB_2IR_Upgrade RGB to 5 model upgrade	1	29231387
AmTyphoon_IP_NIR_Upgrade Add NIR function to IP model upgrade	1	29264465
AmTyphoon_NIR_IP_Upgrade Add IP function to NIR model	1	29264464
AmTyphoon_NIR_GPlus_Upgrade NIR to NIR Plus model upgrade	1	29264467
AmTyphoon_NIR_RGBFluor_Upgrade Add RGB fluorescent function to NIR	1	29264468

Please contact GE Healthcare for additional upgrade combinations.

Optional accessories	Quantity	Product code
Amersham Eraser	1	29187190
Accessory Cabinet AmTyphoon	1	29191637
SlideGlass holder Amersham Typhoon	1	29191521
Cy2(LP) Fltr LPB515 AmTyphoon	1	29191632
Cy3(LP) Fltr LPG550 AmTyphoon	1	29191633
Cy5(LP) Fltr LPR660 AmTyphoon	1	29191634
33 × 42 glass plate guide Amersham Typhoon	1	29215514
Custom filter boxes Amersham Typhoon	1	29191540
Multi-stage AmTyphoon	1	29187198
OD Plate AmTyphoon	1	29191517
Titer plate holder AmTyphoon	1	29191520

Information on upgrade kits for additional lasers, filters, and other items can be obtained by contacting Customer Support.

Related products	Quantity	Product code
Amersham QuickStain	1	RPN4000

CyDye conjugated antibodies

Amersham ECL Plex goat- α -mouse IgG-Cy3, 150 μ g	150 μ g	PA43009
Amersham ECL Plex goat- α -rabbit IgG-Cy3, 150 μ g	150 μ g	28901106

Protein markers

Amersham ECL Plex Fluorescent Rainbow Markers	120 μ l	RPN850E
Amersham ECL Plex Fluorescent Rainbow Markers	500 μ l	RPN851E

Blotting paper

3MM Chr	100 sheets	3030-861
---------	------------	----------

Blotting membranes

Amersham Hybond P 0.45 PVDF 80 mm × 90 mm	25 sheets/PK	10600100
Amersham Hybond LFP 0.2 PVDF 80 mm × 90 mm	25 sheets/PK	10600102
Amersham Protran Premium 0.45 NC 80 mm × 90 mm	25 sheets/PK	10600096

Blocking agent

Amersham ECL™ Prime Blocking Reagent	40 g	RPN418
--------------------------------------	------	--------

Validation support	Quantity	Product code
IQQQ Amersham Typhoon IP	1	29245025
IQQQ Amersham Typhoon RGB	1	29245024
IQQQ Amersham Typhoon 5	1	29145023
IQQQ Amersham Typhoon NIR	1	29288012
IQQQ Amersham Typhoon NIR+	1	29288014

Analysis software	Quantity	Product code
ImageQuant TL, node locked	1	29291744
ImageQuant TL Security, node locked	1	29291745
Melanie 9 Classic Node-locked	1	29270534
Melanie 9 DIGE Node-locked	1	29270536
Melanie 9 Coverage Node-locked	1	29270543



Phosphor screen (Imaging plate)	Quantity	Product code
BAS-IP MS 2040 E <i>Phosphorimaging plate, 20 × 40 cm, multipurpose</i>	1	28956474
BAS-IP MS 2025 E <i>Phosphorimaging plate, 20 × 25 cm, multipurpose</i>	1	28956475
BAS-IP MS 3543 E <i>Phosphorimaging plate, 35 × 43 cm, multipurpose</i>	1	28956476
BAS-IP SR 2040 E <i>Phosphorimaging plate, 20 × 40 cm, high resolution</i>	1	28956477
BAS-IP SR 2025 E <i>Phosphorimaging plate, 20 × 25 cm, high resolution</i>	1	28956478
BAS-IP TR 2040 E <i>Phosphorimaging plate, 20 × 40 cm, for tritium detection</i>	1	28956481
BAS-IP TR 2025 E <i>Phosphorimaging plate, 20 × 25 cm, for tritium detection</i>	1	28956482
BAS-IP ND 2040 E <i>Phosphorimaging plate, 20 × 40 cm, for neutron detection</i>	1	29017133
BAS-IP ND 2025 E <i>Phosphorimaging plate, 20 × 25 cm, for neutron detection</i>	1	29017139
Exposure Cassette, 20 × 25 cm	1	29175523
Exposure Cassette, 35 × 43 cm	1	29175524

The different screens are designed for general use (MS), high resolution suitable for morphological work such as autoradiography (SR), detection of the weak energy of the Tritium signal (TR), and detection of neutron (ND).

Discontinued mounted and unmounted GP phosphor screens are compatible with Amersham Typhoon. These products can be scanned with a Fluor stage (unmounted) and Multi stage (mounted). The Fluor stage and Multi stage are optional accessories for Amersham Typhoon IP.

gelifesciences.com/typhoon

GE, the GE Monogram, Amersham, Cy, CyDye, DaTscan, ECL Plex, ExcelGel, ImageQuant, Hybond, Protran, and Typhoon are trademarks of General Electric Company. Alexa Fluor and SYPRO are trademarks of Life Technologies Corporation. Coomassie and DyLight are trademarks of Thermo Fisher Scientific LLC. Intel is a trademark of Intel Corporation. IRDye is a trademark of LI-COR, Inc. Melanie is a trademark of SIB Swiss Institute of Bioinformatics. Windows is a registered trademark of Microsoft Corporation. All other third-party trademarks are the property of their respective owner. 2D-DIGE: 2D Fluorescence Difference Gel Electrophoresis (2D-DIGE) technology is covered by US patent number 6,127,134 and equivalent patents and patent applications in other countries and exclusively licensed from Carnegie Mellon University.

The purchase of CyDye DIGE Fluors includes a limited license to use the CyDye DIGE Fluors for internal research and development, but not for any commercial purposes. A license to use the CyDye DIGE Fluors for commercial purposes is subject to a separate license agreement with GE Healthcare.

CyDye: The purchase of CyDye products includes a limited license to use the CyDye products for internal research and development but not for any commercial purposes. A license to use the Cy and CyDye trademarks for commercial purposes is subject to a separate license agreement with GE Healthcare. Commercial use shall include:

1. Sale, lease, license or other transfer of the material or any material derived or produced from it.
2. Sale, lease, license or other grant of rights to use this material or any material derived or produced from it.
3. Use of this material to perform services for a fee for third parties, including contract research and drug screening.

If you require a commercial license to use the Cy and CyDye trademarks please contact LSlicensing@ge.com.

© 2018 General Electric Company

All goods and services are sold subject to the terms and conditions of sale of the company within GE Healthcare which supplies them.

A copy of these terms and conditions is available on request. Contact your local GE Healthcare representative for the most current information.

GE Healthcare UK Ltd., Amersham Place, Little Chalfont, Buckinghamshire, HP7 9NA, UK

GE Healthcare Europe GmbH, Munzinger Strasse 5, D-79111 Freiburg, Germany

GE Healthcare Bio-Sciences Corp., 100 Results Way, Marlborough, MA 01752, USA

GE Healthcare Japan Corp., Sanken Bldg., 3-25-1, Hyakunincho Shinjuku-ku, Tokyo 169-0073, Japan

GE Healthcare Bio-Sciences AB, Björkgatan 30, 751 84 Uppsala, Sweden

For local office contact information, visit www.gelifesciences.com/contact.

KA1285051018DF