

Make your first attempt your best. Every time.

You do your best to avoid airway complications. You know they can be associated with significant patient morbidity and unnecessary expense.¹⁻³ But sometimes they occur when you least expect them.^{4,5}

With the McGRATH™ MAC video laryngoscope, you can be better prepared for the unexpected.

Combining confidence with simplicity and convenience, it provides:

- Better glottic visualization than traditional Macintosh laryngoscopy⁶
- Higher intubation success rates than many other video laryngoscopes⁷
- May be associated with less hemodynamic stimulation than direct laryngoscopy and certain video laryngoscopes.⁸⁻¹⁰

A FAMILIAR TECHNIQUE — EVOLVED


The McGRATH™ MAC video laryngoscope combines line-of-sight video from its portrait display with the familiar Macintosh technique. So you retain your traditional laryngoscopy skills.

SIMPLE, SMART, AND VERSATILE

The single-button functionality and minute-by-minute battery indication and auto shut off feature to optimize battery life. One handle with multiple blade options. From pediatric to adult patients and routine to extreme airways.¹¹⁻¹³

DESIGNED FOR ROUTINE USE

The McGRATH™ MAC is durable and designed to endure fast-paced hospital and EMS environments.



ORDERING INFORMATION

SKU NO.	DESCRIPTION	QUANTITY
301-000-000	McGRATH™ MAC handle	1
350-072-000	McGRATH™ MAC blade size 1	50/box
350-017-000	McGRATH™ MAC blade size 2	50/box
350-005-000	McGRATH™ MAC blade size 3	50/box
350-013-000	McGRATH™ MAC blade size 4	50/box
X3-003-000	McGRATH™ MAC X blade size 3	10/box
340-000-000	Battery pack, 250-minute	1

TECHNICAL SPECIFICATIONS


McGRATH™ MAC handle

Size	180 mm x 68 mm x 110 mm
Weight	180 g
Power	3.6V lithium battery pack (c. 250 minutes)
Light source	High-intensity LED
Display	2.5" LCD color display
Camera	CMOS
Materials	Durable medical-grade thermoplastics composite with structural alloy core. The device and packaging are latex free.
Warranty	36 months

McGRATH™ MAC disposable blades

Material	Fog-free medical-grade optical polymer
Packaging	Packaged sterile for single use

For demonstrations and quotes, please contact your local representative.
Find out more at medtronic.com/mac-first

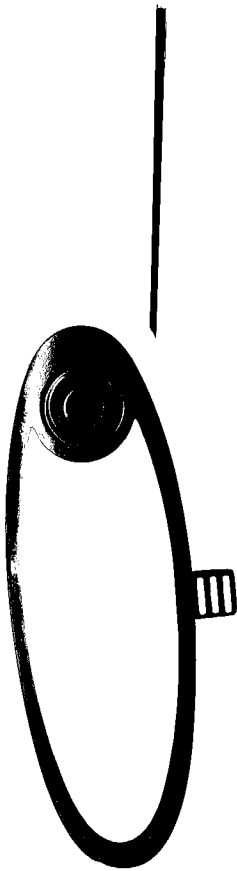

X blade size 3



Macintosh
Blade size 4



Macintosh
Blade size 3



Macintosh
Blade size 2



Macintosh
Blade size 1



1. Faccio JE, Nishisaki A, Jagannathan N, et al. Airway management complications in children with difficult tracheal intubation from the Pediatric Difficult Intubation (PeDi) registry: a prospective cohort analysis. *Lancet Respir Med*. 2016;4(1):57-68.
2. Metzner J, Posner KL, Lam MS, Domino KB. Closed claims analysis. *Best Pract Res Clin Anaesthesiol*. 2011;25(2):265-276.
3. Cook T, Woodall N, Frerk C. 4th National Audit Project of the Royal College of Anaesthetists and The Difficult Airway Society: Major complications of airway management in the United Kingdom. <http://www.coa.ac.uk/system/files/CSQ-NAP4-Ful.pdf>. Published March 2011. Accessed January 2017.
4. Nersisyan AK, Rosenstock CV, Westerslev J, Astrup G, Afshar A, Lundström LH. Diagnostic accuracy of anaesthesiologists' prediction of difficult airway management in daily clinical practice: a cohort study of 188 064 patients registered in the Danish Anaesthesia Database. *Anaesthesia*. 2015;70(5):272-281.
5. Hutink JM, Lo PP, Heiderman I, et al. A prospective, cohort evaluation of major and minor airway management complications during routine anaesthetic care at an academic medical centre. *Anaesthesia*. 2017;72(1):42-48.
6. Shin M, Bai S, Lee KY, Oh E, Kim H. Comparing McGrath-MAC, C-MAC®, and Macintosh laryngoscopes operated by medical students: a randomized, crossover, manikin study. *Bioméd Res Int*. 2016;2016:8945951.
7. Kleire-Brueggemann M, Gref R, Schoettke P, Savolcell GL, Naboecker S, Theiler LG. Evaluation of six video laryngoscopes in 20 patients with a simulated difficult airway: a multicentre randomized controlled trial. *Br J Anaesth*. 2016;116(5):670-679.
8. Bunari FS, Selveraj V. Randomized controlled study comparing the hemodynamic response to laryngoscopy and endotracheal intubation with McCoy, Macintosh, and C-MAC laryngoscopes in adult patients. *Journal Of Anaesthesiology, Clinical Pharmacology*. 2016;32(4):505-509. doi:10.4103/0970-9185.194766.
9. Coak F, Ozgul J, Erdogan MA, et al. Comparison of hemodynamic responses and QTc intervals to tracheal intubation with the McGrath MAC videolaryngoscope and the Macintosh direct laryngoscope in elderly patients. *The Kaohsiung Journal Of Medical Sciences*. 2019;35(2):116-122. doi:10.1002/kjms.12017.
10. Altun D, Al A, Çamaç E, Özoruç A, Seymen TC. Haemodynamic Response to Four Different Laryngoscopes. *Turkish Journal Of Anaesthesiology And Reanimation*. 2018;46(6):434-440. doi:10.5152/TJAR.2018.59265.
11. Gaszynski T. Comparison of the gottlieb view during video-intubation in super-obese patients: a series of cases. *Thor Clin Risk Manag*. 2016;12:167-1682.
12. Szarpak L, Tuszyński Z, Czyżewski J, Gaszynski T, Rodriguez-Nuñez A. A comparison of the McGrath-MAC and Macintosh laryngoscopes for child tracheal intubation during resuscitation by paramedics: a randomized, crossover, manikin study. *Am J Emerg Med*. 2016;34(8):1338-1341.
13. Ross M, Baxter A. Use of the new McGrath MAC size-1 paediatric videolaryngoscope. *Anaesthesia*. 2015;70(10):1217-1218.

© 2017, 2018, 2019 Medtronic. All rights reserved. Medtronic, Medtronic logo and Further. Together are trademarks of Medtronic. All other brands are trademarks of a Medtronic company. 10/2019-15-AW-0056(4)-[WF#2927481]