



Smlouva o výpůjčce

č. 1344/2018/ÚVN

Smluvní strany:

CARDION s.r.o.

zapsaná v obchodním rejstříku vedeném U Krajského soudu v Brně, oddíl C, vložka 16405

se sídlem: Rybnická 257/136, 634 00, Brno

zastoupená: Ing. Ivo Nekudou

IČ: 60719877

DIČ: CZ699003452

bankovní spojení:

dále jen „**půjčitel**“

a

Ústřední vojenská nemocnice – Vojenská fakultní nemocnice Praha

príspevková organizace zřízená Ministerstvem obrany ČR

se sídlem: U Vojenské nemocnice 1200, 169 02 Praha 6

IČO: 61383082

DIČ: CZ61383082

bankovní spojení:

zastoupená: prof. MUDr. Miroslavem Zavoralem, Ph.D., ředitelem

dále jen „**vypůjčitel**“

uzavírají dle zákona č. 89/2012 Sb., občanský zákoník, v platném znění, a za podmínek níže stanovených, tuto smlouvu o výpůjčce:

I.

Půjčitel je výlučným vlastníkem věci: QUANTIEM – FFR měřicí systém, v pořizovací hodnotě 152.893,- Kč bez DPH.

Specifikace věci: výrobce St. Jude Medical, výrobní č. Q00501 typ: QUANTIEN C12787

(dále jen „**přístroj**“)

II.

1. Půjčitel touto smlouvou přenechává bezplatně přístroj uvedený v předchozím článku do užívání vypůjčiteli, který jej přijímá do výpůjčky.
2. Půjčitel prohlašuje, že přístroj je nový a nepoužitý.
3. Přístroj bude umístěn v sídle vypůjčitele na Interní klinice 1. LF UK a ÚVN, Oddělení invazivní kardiologie a arytmologie, v Ústřední vojenské nemocnici – Vojenské fakultní nemocnici Praha.
4. Půjčitel se zavazuje, že o plánovaném termínu předání a převzetí přístroje bude kontaktovat Oddělení zdravotnické techniky vypůjčitele (dále jen „OZT“) nejméně 2 dny předem.
5. Odpovědnými osobami za předání a převzetí přístroje jsou:

III.

1. Půjčitel se zavazuje přístroj předat vypůjčiteli, a umístit jej na pracovišti vypůjčitele, o čemž obě smluvní strany sepíší zápis.
2. Spolu s přístrojem, který je zdravotnickou technikou ve smyslu zákona č. 268/2014 Sb., o zdravotnických prostředcích a o změně zákona č. 634/2004 Sb., o správních poplatcích, ve znění

pozdějších předpisů, bude předáno též prohlášení o shodě a návod k použití v českém jazyce v listinné a elektronické podobě.

3. Půjčitel je povinen předat vypůjčiteli přístroj ve stavu způsobilém k řádnému užívání. Půjčitel se zavazuje provést na své náklady zaškolení odpovědných zaměstnanců vypůjčitele v obsluze přístroje, o čemž bude vystaven písemný doklad, tj. protokol o zaškolení.
4. Půjčitel se dále zavazuje zajistit bezplatně po dobu trvání výpůjčky pravidelné školení odpovědných zaměstnanců vypůjčitele v obsluze přístroje alespoň jedenkrát ročně na základě písemného požadavku vypůjčitele.
5. Vypůjčitel je povinen užívat přístroj řádně a v souladu s účelem, ke kterému je přístroj určen. Vypůjčitel je povinen chránit přístroj před jakýmkoli poškozením, ztrátou nebo zničením.
6. Vypůjčitel nese odpovědnost pouze za škody na přístroji způsobené užíváním, které není v souladu s účelem, ke kterému je přístroj určen. Půjčitel je oprávněn smlouvu okamžitě vypovědět, jestliže vypůjčitel věc užívá v rozporu s touto smlouvou.
7. Půjčitel se zavazuje, že po dobu vypůjčení přístroje zajistí bezplatný servis, opravy a validaci (bezpečnostně technickou kontrolu) přístroje včetně veškerého potřebného spotřebního materiálu (vyměňovaného při opravách – nikoliv provozního spotřebního materiálu), a to vždy ve lhůtě 48 hodin od nahlášení potřeby opravy vypůjčitelem. Půjčitel se dále zavazuje pro případ dlouhodobé opravy (více než 72 hodin od nahlášení potřeby opravy vypůjčitelem) zapůjčit vypůjčiteli jiný přístroj stejného typu zdarma. Pokud však závadu na přístroji způsobil vypůjčitel porušením svých povinností stanovených touto smlouvou, hradí veškeré náklady spojené s opravou přístroje vypůjčitel.
8. Půjčitel se zavazuje, že veškerou dokumentaci o činnostech provedených na přístroji v době trvání výpůjčky (např. protokoly BTK a servisní výkazy) předá neprodleně na OZT.
9. Půjčitel se zavazuje provádět upgrade softwaru přístroje.
10. Půjčitel se zavazuje pojistit přístroj na dobu jeho vypůjčení na vlastní náklady.
11. Vypůjčitel nesmí přenechat přístroj k užívání třetí osobě.

IV.

1. Výpůjčka se sjednává **po dobu trvání Kupní smlouvy na dodávku spotřebního zdravotnického materiálu pro vyšetření Frakční průtokové rezervy uzavřené dne^{29.8.2018} a v souladu s touto kupní smlouvou.**
2. Tato smlouva zanikne dnem, ve kterém zanikne kupní smlouva uvedená v odst.1.
3. Vypůjčitel je povinen vrátit přístroj půjčiteli, jakmile jej přestane potřebovat, nejpozději však do konce doby výpůjčky. Půjčitel se zavazuje, že v takovém případě převezme na výzvu vypůjčitele přístroj v sídle vypůjčitele, a to do 5 dnů od vyzvání vypůjčitelem. Půjčitel si přístroj odveze na své náklady.

V.

1. Tato smlouva nabývá platnosti a účinnosti dnem podpisu oběma smluvními stranami, není-li dále stanoveno jinak.
2. V případě, že smlouva podléhá povinnému uveřejnění v registru smluv podle zákona č. 340/2015 Sb., o zvláštních podmínkách účinnosti některých smluv, uveřejňování těchto smluv a o registru smluv (zákon o registru smluv), v platném znění (hodnota přístroje vyšší než 50.000,- Kč bez DPH), souhlasí smluvní strany s tím, že smlouvu zašle správci registru smluv k uveřejnění vypůjčitel, a to do 10 pracovních dnů od jejího uzavření. Obě smluvní strany prohlašují, že žádnou část této smlouvy nepovažují za své obchodní tajemství.
3. Tuto smlouvu lze měnit a doplňovat jen písemnými dodatky číslovanými vzestupnou, nepřerušovanou číselnou řadou.
4. Tato smlouva je vyhotovena ve **dvou stejnopisech**, z nichž každá ze smluvních stran obdrží po jednom.

Nedílná příloha této smlouvy:

- Příloha č. 1 – Technická specifikace přístroje – datasheety, produktové listy, katalogy, atp.

V Brně dne 9. 8. 2018

29 -08- 2018

V Praze dne

za půjčitele:

za vypůjčitele:

V ZASTOUPENÍ

MUDr. Ivan Jeřábek
náměstek ředitele pro LPP ÚVN

Ing. Ivo NEKUDA
jednatel společnosti CARDION s.r.o.

CARDION s.r.o.
Rybnická 136, 634 09 Brno
Tel: 547 241 313
IČO: 00719877
EPH DIČ: CZ699003452

prof. MUDr., Ph.D.
ředitel Ústřední vojenské nemocnice –
Vojenské lékařské nemocnice Praha



TECHNICKÝ POPIS


FFR – Měřicí systém QUANTIEN™

Objednávkový kód: C12787

QUANTIEN Measurement System je tvořen diagnostickým počítačem, určeným k záznamu, výpočtu, zobrazení a ukládání dat z vodícího drátu PressureWire™, a dalších externích snímačů. Informace jsou zobrazeny v podobě grafů i číselných hodnot na obrazovce. Mezi snímané hodnoty patří: systolický, diastolický a střední tlak krve, srdeční tep, frakční průtoková rezerva (FFR) a data z ECG.

Informace na obrazovce lze také přenášet do externího hemodynamického záznamového systému nebo na externí monitor. Zaznamenávané zákroky lze pro následnou kontrolu a analýzu zobrazit na počítači pomocí nainstalovaného zobrazovacího softwaru konkrétní aplikace, např. RadiView™. Další funkce vám umožní importovat seznam úloh u pacienta z nemocničního systému DICOM, export naměřené a zaznamenané hodnoty do systému DICOM nebo na externí server, popř. je uložit na USB paměťový disk.

QUANTIEN Measurement System je určen k použití v katetrizačních a podobných specializovaných kardiovaskulárních laboratořích pro výpočet a zobrazení různých fyziologických parametrů na základě výstupů z jedné nebo několika elektrod, snímačů nebo měřicích přístrojů.

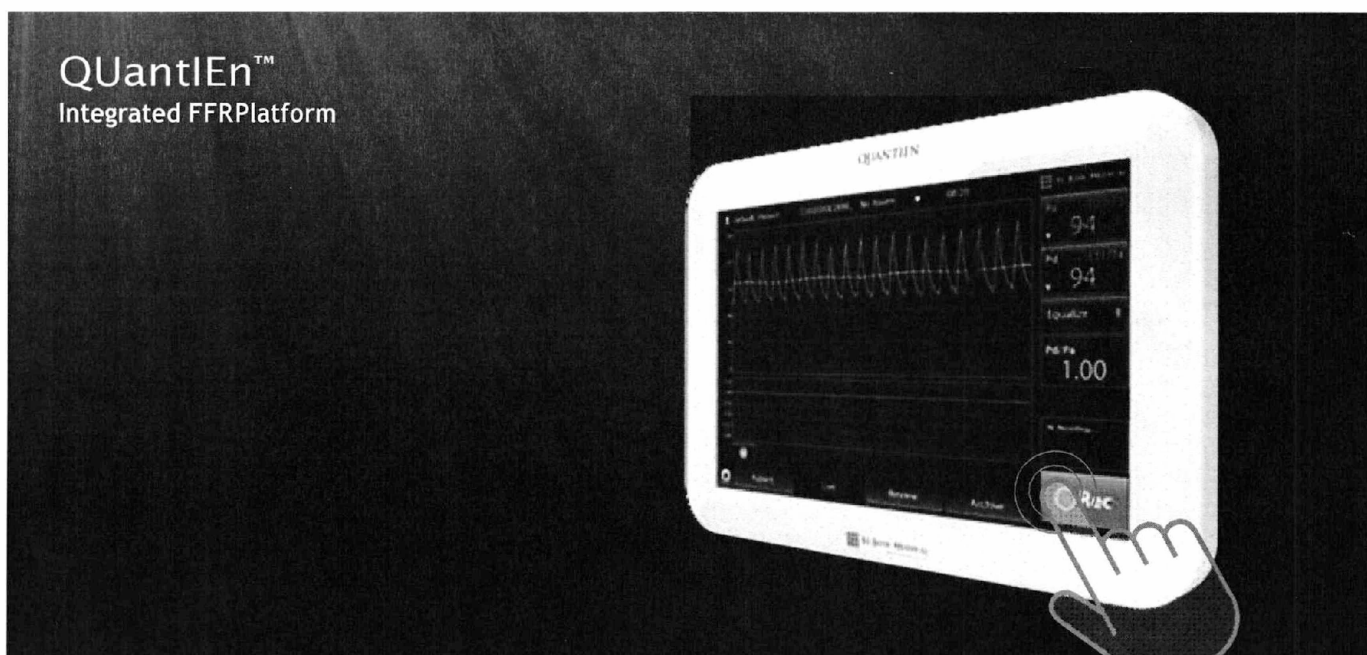

INTRODUCING
QUANTIEN™

Integrated FFR Platform

FREE YOUR CATH LAB WITH WIRELESS FFR




ST. JUDE MEDICAL
MORE CONTROL. LESS RISK.

QUANTIEN

FREE YOUR CATH LAB WITH WIRELESS

Free from Cables

The QUANTIEN integrated FFR solution gives you a wireless patient environment, removing the clutter of cables and clearing the table for what's most important — the patient.

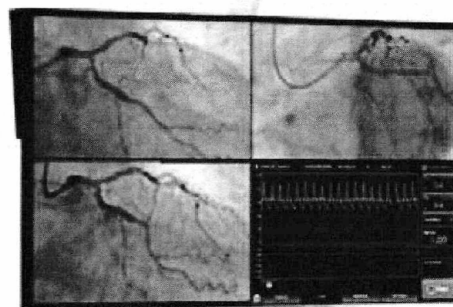

FFR screen on existing monitors

Free Up Your Time

With QUANTIEN, FFR is always available when and where you want it, without time-consuming setup or connecting of cables. Patient ID is quickly loaded from your hospital scheduling system, and the results are exported back to your archive, all with a minimum of manual interaction.



Wi-Box™
Wireless AO Interface



Perfect Touch Display


All features at your fingertips through the latest touch-screen technology and a high-resolution widescreen.




Full Connectivity

Quick and easy procedures and full case documentation with DICOM worklist, DICOM archive and USB memory stick data export.

FFR

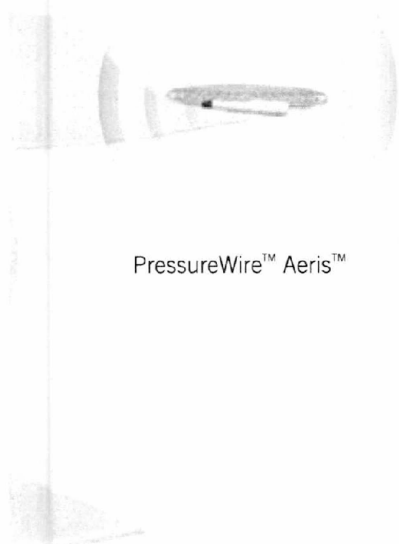

PressureWire™ Aeris™

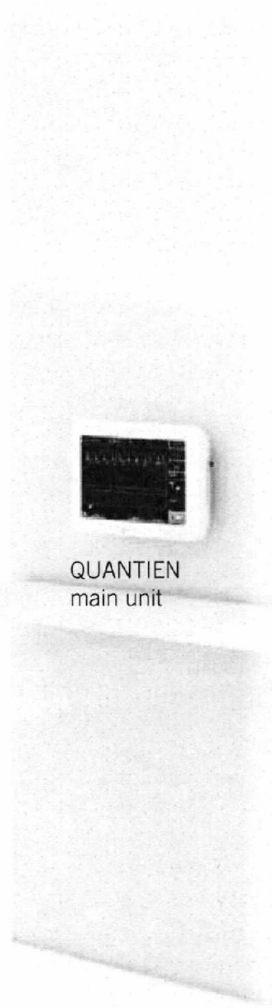

QUANTIEN
main unit

Free Your Table

The wireless design of the QUANTIEN integrated FFR solution allows you to tailor your cath lab environment exactly the way you like. Place the QUANTIEN main unit anywhere in the lab, freeing up valuable table space and allowing control by either sterile or nonsterile-dressed staff.

Regardless of where you chose to place QUANTIEN, its video screen can be displayed on existing lab monitors for convenient viewing right next to your angiography and hemodynamic screens.

Free from Time-Consuming Installation

Integrating QUANTIEN into your cath lab environment is quick and easy — no need to install cables through the floor or ceiling. QUANTIEN lets you go wireless without taking down the lab.



Secure Wireless

Fast, robust and secure wireless communication using advanced radio technology from St. Jude Medical. Well proven in cath labs around the world.




PressureWire

The Quantien integrated FFR platform is compatible with PressureWire Certus™ and PressureWire Aeris from St. Jude Medical.


WIRELESS FFR. LIGHT YEARS AHEAD




Solutions for
PCI Optimization

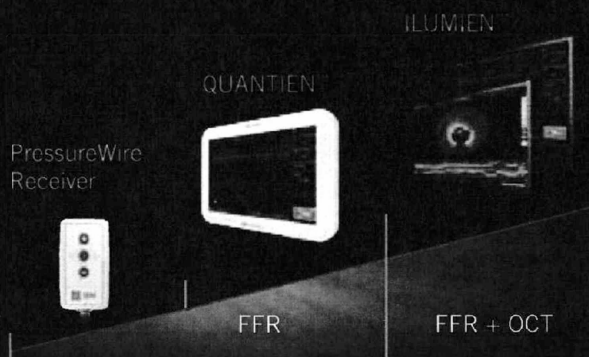

Guided Procedures

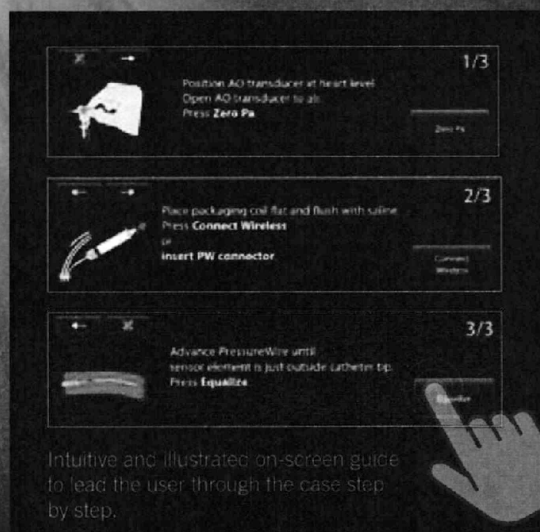


Multivessel FFR Made Easy

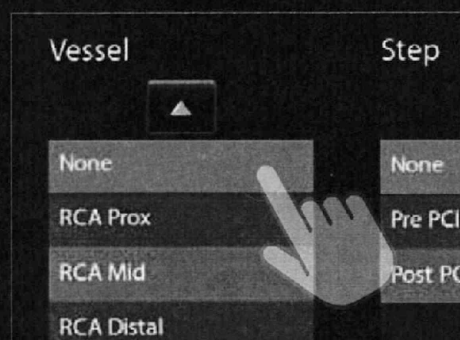

Simplified live case documentation with vessel and procedure step annotation.

Get Your Data in Seconds

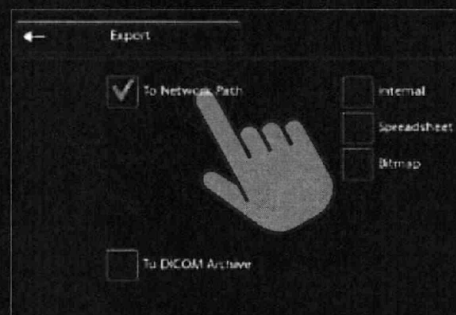

Fast and easy data export via USB memory stick or network.

Our Claim to FAME and FAME 2

FAME

Compared to angiography alone, FFR¹:

- Allows more accurate identification of hemodynamically relevant stenoses, reducing rates of death, myocardial infarction and repeat revascularization¹
- Improves outcomes and patient quality of life
- Lowers procedure-related costs
- No increase in procedure time
- Decreases the amount of contrast agent used

FAME 2

FFR-guided PCI using PressureWire is a cost-effective strategy that improves outcomes and quality of life compared to medical therapy alone.²⁻³

- 86% relative reduction in the risk for ACS requiring unplanned hospital readmission with urgent revascularization
- Greater relief of angina
- Cost-effectiveness – ICER of \$32,000 per QALY

Ordering Information

Model / Reorder Number	Product
C12787	QUANTIEN FFR Plattform
C12797	QUANTIEN Desktop stand
C12798	QUANTIEN Pole bracket
C12799	QUANTIEN Wall mount
C12783	Wi-Box

Note: To fasten QUANTIEN bedside with no bedside mounted pole available, order Multipurpose Bracket C12777 and C12798 Pole Bracket.

1. Tonino PA, De Bruyne B, Pijls NH, et al. Fractional flow reserve versus angiography for guiding percutaneous coronary intervention. *FAME study*. *N Engl J Med*. 2009;360(3):213-24.
2. De Bruyne B, Pijls N, Kalesan B, et al. Fractional flow reserve-guided PCI versus medical therapy in stable coronary disease. *N Engl J Med*. 2012;367(11):991-1001.
3. Fearon WF. FAME 2 Cost-effectiveness: A Prospective, Randomized Trial Evaluating the Cost-effectiveness of FFR-Guided PCI in Patients with Stable Coronary Artery Disease Presented at Late Breaking Clinical Trials 1 at TCT 2012, Miami, Florida, October 24, 2012.

ATRIAL FIBRILLATION

CARDIAC RHYTHM MANAGEMENT

CARDIOVASCULAR

NEUROMODULATION

Global Headquarters

One St. Jude Medical Drive
St. Paul, Minnesota 55117
USA
+1 651 756 2000
+1 651 756 3301 Fax

Cardiovascular Division

177 East County Road B
St. Paul, Minnesota 55117
USA
+1 651 756 4470
+1 651 756 4466 Fax

St. Jude Medical Systems AB

Box 6350
SE-751 35 Uppsala
Sweden
+46 18 161000
+46 18 161099 Fax

SJM Coordination Center BVBA

The Corporate Village
Da Vincilaan 11 Box F1
1935 Zaventem, Belgium
+32 2 774 68 11
+32 2 772 83 84 Fax

St. Jude Medical Japan Co., Ltd.

Shiodome City Center 15F
1-5-2, Higashi-Shinbashi, Minato-ku
Tokyo 105-7115
Japan
+81 3 6255 6370
+81 3 6255 6371 Fax

St. Jude Medical (Hong Kong) Ltd.

Suite 1608, 16/F Exchange Tower
33 Wang Chiu Road
Kowloon Bay, Kowloon
Hong Kong SAR
+852 2996 7688
+852 2956 0622 Fax

St. Jude Medical Brasil Ltda.

Rua Itapeva, 538
5º ao 8º andar
01332-000 – São Paulo (SP)
Brazil
+55 11 5080 5400
+55 11 5080 5423 Fax

St. Jude Medical Australia Pty. Ltd.

17 Orion Road
Lane Cove, NSW 2066
Australia
+61 2 9936 1200
+61 2 9936 1222 Fax

SJMprofessional.com

SJMknowledgecenter.com



ST. JUDE MEDICAL
MORE CONTROL. LESS RISK.

Product referenced is approved for CE Mark.

Not available for sale in the U.S. Devices depicted may not be available in all countries. Check with your St. Jude Medical representative for product availability in your country.

Please review the Instructions for Use prior to using these devices for a complete listing of indications, contraindications, warnings, precautions, potential adverse events and directions for use.

QUANTIEN, PressureWire Aegis, PressureWire Certus and Wi-Box are designed, developed and manufactured by St. Jude Medical Systems AB. QUANTIEN, ILUMIEN, PRESSUREWIRE, AERIS, CERTUS, WI-BOX, RADI, ST. JUDE MEDICAL, the nine-squares symbol and MORE CONTROL. LESS RISK. are registered and unregistered trademarks and service marks of St. Jude Medical, Inc. and its related companies.


©2012 St. Jude Medical, Inc. All rights reserved.

GMVASC471EN

IPN 2342-12



QUANTIEN™
Integrated FFR Platform

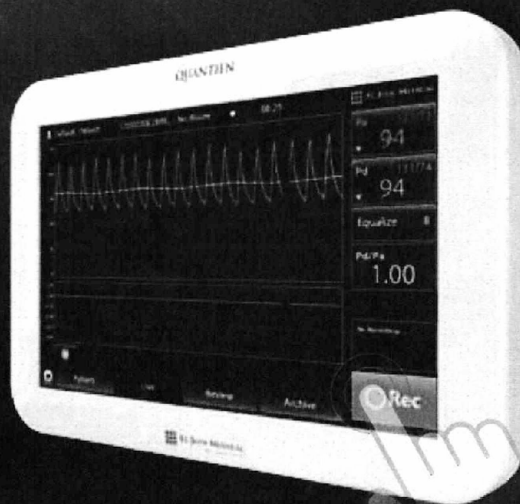

FREE YOUR CATH LAB WITH WIRELESS FFR FAST AND EASY FFR INTEGRATION

The wireless design of the QUANTIEN integrated FFR platform allows you to configure your cath lab environment exactly the way you like – without the clutter of cables.

Easy cath lab installation gives you full FFR integration without cabling through floor or ceiling – and without cath lab downtime.

With the wireless Wi-Box™ and PressureWire™ Aeris™, the QUANTIEN main unit can be placed as a built-in or mobile device anywhere in the cath lab, freeing up valuable table space and allowing control by either sterile- or nonsterile-dressed staff.

FAST AND EASY WIRELESS FFR

With QUANTIEN, FFR is always available when and where you want it, without time-consuming setup or cables.

EASY TO PLACE

Place it where you want it – on a desktop, on a wall, bedside or on a mobile pole.

FULL VISIBILITY

Regardless of where you place the QUANTIEN main unit, you can view its video screen on the existing cath lab monitors right next to your angio and hemo screens.

TOUCH DISPLAY

You have fingertip access to all features, using the latest touch screen technology and a high-resolution widescreen.

FULL CONNECTIVITY

Quick and easy procedures and full case documentation with DICOM Worklist, DICOM Archive, local network and USB memory stick data export.



ST. JUDE MEDICAL®
MORE CONTROL. LESS RISK.


Ordering Information

QUANTIEN

Model/Reorder Number	Description
C12787	QUANTIEN FFR Plattform
C12797	QUANTIEN Desktop stand
C12798	QUANTIEN Pole bracket
C12799	QUANTIEN Wall mount

Note: To fasten QUANTIEN bedside with no bedside mounted pole available, order Multipurpose Bracket C12777 and C12798 Pole Bracket.

Solutions for PCI Optimization

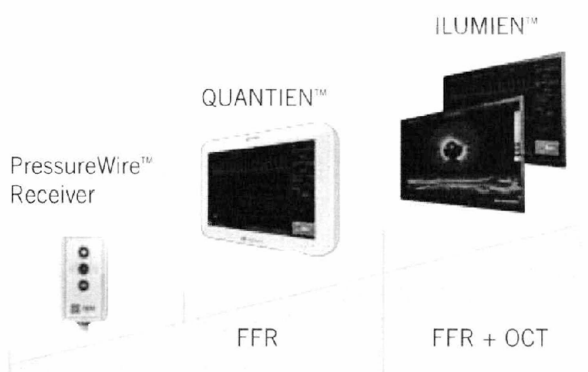

ATRIAL FIBRILLATION

CARDIAC RHYTHM MANAGEMENT

CARDIOVASCULAR

NEUROMODULATION

Global Headquarters

One St. Jude Medical Drive
St. Paul, Minnesota 55117
USA
+1 651 756 2000
+1 651 756 3301 Fax

Cardiovascular Division

177 East County Road B
St. Paul, Minnesota 55117
USA
+1 651 756 4470
+1 651 756 4466 Fax

St. Jude Medical Systems AB

Box 6350
SE-751 35 Uppsala
Sweden
+46 18 161000
+46 18 161099 Fax

SJM Coordination Center BVBA

The Corporate Village
Da Vincilaan 11 Box F1
1935 Zaventem, Belgium
+32 2 774 68 11
+32 2 772 83 84 Fax

St. Jude Medical Japan Co., Ltd.

Shiodome City Center 15F
1-5-2, Higashi-Shinbashi, Minato-ku
Tokyo 105-7115
Japan
+81 3 6255 6370
+81 3 6255 6371 Fax

St. Jude Medical (Hong Kong) Ltd.

Suite 1608, 16/F Exchange Tower
33 Wang Chiu Road
Kowloon Bay, Kowloon
Hong Kong SAR
+852 2996 7688
+852 2956 0622 Fax

St. Jude Medical Brasil Ltda.

Rua Itapeva, 538
5º ao 8º andar
01332-000 – São Paulo (SP)
Brazil
+55 11 5080 5400
+55 11 5080 5423 Fax

St. Jude Medical Australia Pty. Ltd.

17 Orion Road
Lane Cove, NSW 2056
Australia
+61 2 9936 1200
+61 2 9936 1222 Fax

SJMprofessional.com

SJMknowledgecenter.com



ST. JUDE MEDICAL

MORE CONTROL. LESS RISK.

Product referenced is approved for CE mark.

Not available for sale in the U.S. Devices depicted may not be available in all countries. Check with your St. Jude Medical representative for product availability in your country.

Please review the Instructions for Use prior to using these devices for a complete listing of indications, contraindications, warnings, precautions, potential adverse events and directions for use.



QUANTIEN, PressureWire Aegis and Wi-Box are designed, developed and manufactured by St. Jude Medical Systems AB. QUANTIEN, PressureWire, Aegis, Wi-Box, ILUMIEN, RADI, ST. JUDE MEDICAL, the nine-squares symbol and MORE CONTROL. LESS RISK. are registered and unregistered trademarks and service marks of St. Jude Medical, Inc. and its related companies. ©2012 St. Jude Medical, Inc. All rights reserved.

Item GMVASC472EN IPN 2378-12



QUANTIEN™

Integrated FFR Platform



SPECIFICATIONS

HEIGHT X DEPTH X WIDTH

Main Unit:	260 x 100 x 375 mm
Shipment box:	393 x 170 x 493 mm

SCREEN SIZE

Touch screen size:	14.1 inch
--------------------	-----------

WEIGHT

With transformer:	4.8 kg incl. PSU, PWI and PWI cable
-------------------	-------------------------------------

OPERATING VOLTAGE

100-240VAC 50/60Hz

ENVIRONMENT

Operating temperature:	15 °C to 35 °C (59 °F to 95 °F)
Relative humidity, operating:	30 % - 75 %
Ambient pressure, operating:	525-795 mmHg (700-1060 mbar)

COOLING SYSTEM

Passive, no fan

ETHERNET

Type:	10/100 Mbit/s
Connector:	RJ45

VIDEO OUT

Frequency:	60Hz
Resolution:	1280x800
Connector:	DVI-I (integrated - digital and analog)

USB

Number:	1
Version:	2.0, supports Hi-speed communication
Connector:	Type A, Receptacle

MOUNTING

VESA :	75x75 mm and 100x100 mm
	Specific mounting brackets available for ordering from St. Jude Medical

AUX 1 IN (AO)

Differential analog input	
Scale factor:	Selectable between 50 mmHg/V and 200 mmHg/V
Range:	+/- 10 V
Isolation:	IEC 60601-1 Basic isolation

AUX 2 IN (ECG)

Differential analog input	
Scale factor:	1 mV / V
Range:	± 10 V
Isolation:	IEC 60601-1 Basic isolation

AUX OUT 1 AND 2

Analog output	
Signal source:	Selectable Pa or Pd
Scale factor:	1 V / 100 mmHg
Isolation:	IEC 60601-1 Basic isolation

PRESSURE SPECIFICATION

Pressure range:	-30 to 300 mmHg
Pressure resolution:	0.2 mmHg
Frequency response:	0-25 Hz

ACCURACY

Pressurewire:	-30 to 300 mmHg ± 1 mmHg plus ±1 % reading (over the pressure range -30 to 50 mmHg) ± 3 % of reading (over the range 50 to 300 mmHg)
---------------	--

The accuracy is given for the combination of QUANTIEN and PressureWire

AUX IN 1 (AO):	± 1 mmHg or 0.5 %, whichever is greatest
Wi-Box (AO):	± 1 mmHg or 1 %, whichever is greatest

WIRELESS TRANSMISSION

Frequency:	2.4 GHz ISM band
Type:	Frequency Hopping Spread spectrum (FHSS)

ORDERING INFORMATION

Model/Reorder Number	Description
C12787	QUANTIEN FFR Platform
C12797	QUANTIEN Desktop stand
C12798	QUANTIEN Pole bracket
C12799	QUANTIEN Wall mount

Note: To fasten QUANTIEN bedside with no bedside mounted pole available, order Multipurpose Bracket C12777 and C12798 Pole Bracket.



ST. JUDE MEDICAL™
MORE CONTROL LESS RISK

ATRIAL FIBRILLATION

CARDIAC RHYTHM MANAGEMENT

CARDIOVASCULAR

NEUROMODULATION

Global Headquarters

One St. Jude Medical Drive
St. Paul, Minnesota 55117
USA
+1 651 756 2000
+1 651 756 3301 Fax

Cardiovascular Division

177 East County Road B
St. Paul, Minnesota 55117
USA
+1 651 756 4470
+1 651 756 4466 Fax

St. Jude Medical Systems AB

Box 6350
SE-751 35 Uppsala
Sweden
+46 18 161000
+46 18 161099 Fax

St. Jude Medical Brasil Ltda.

Rua Itapeva, 538
5º ao 8º andar
01332-000 – São Paulo – SP
Brazil
+55 11 5080 5400
+55 11 5080 5423 Fax

SJM Coordination Center BVBA

The Corporate Village
Avenue Da Vincilaan 11 Box F1
B-1935 Zaventem, Belgium
+32 2 774 68 11
+32 2 772 83 84 Fax

St. Jude Medical Japan Co., Ltd.

Shiodome City Center 15F
1-5-2, Higashi-Shinbashi
Minato-ku, Tokyo 105-7115
Japan
+81 3 6255 6370
+81 3 6255 6371 Fax

St. Jude Medical (Hong Kong) Ltd.

Suite 1608, 16/F Exchange Tower
33 Wang Chiu Road
Kowloon Bay, Kowloon
Hong Kong SAR
+852 2996 7688
+852 2956 0622 Fax

St. Jude Medical Australia Pty Ltd.

17 Orion Road
Lane Cove NSW 2066
Australia
+61 2 9936 1200
+61 2 9936 1222 Fax

SJMprofessional.com

SJMknowledgecenter.com



ST. JUDE MEDICAL

MORE CONTROL. LESS RISK.

Product referenced is approved for CE mark.

Not available for sale in the U.S. Devices depicted may not be available in all countries. Check with your St. Jude Medical representative for product availability in your country.

Please review the Instructions for Use prior to using these devices for a complete listing of indications, contraindications, warnings, precautions, potential adverse events and directions for use.

Quantien, PressureWire and Aeris are designed, developed and manufactured by St. Jude Medical Systems AB. QUANTIENT, PressureWire, Aeris, ST. JUDE MEDICAL, the nine-squares symbol and MORE CONTROL. LESS RISK. are registered and unregistered trademarks and service marks of St. Jude Medical, Inc. and its related companies.

©2012 St. Jude Medical, Inc. All rights reserved.

IPN 2343-12 Item GMVASC464EN

